



1 / 16

Fig. 1

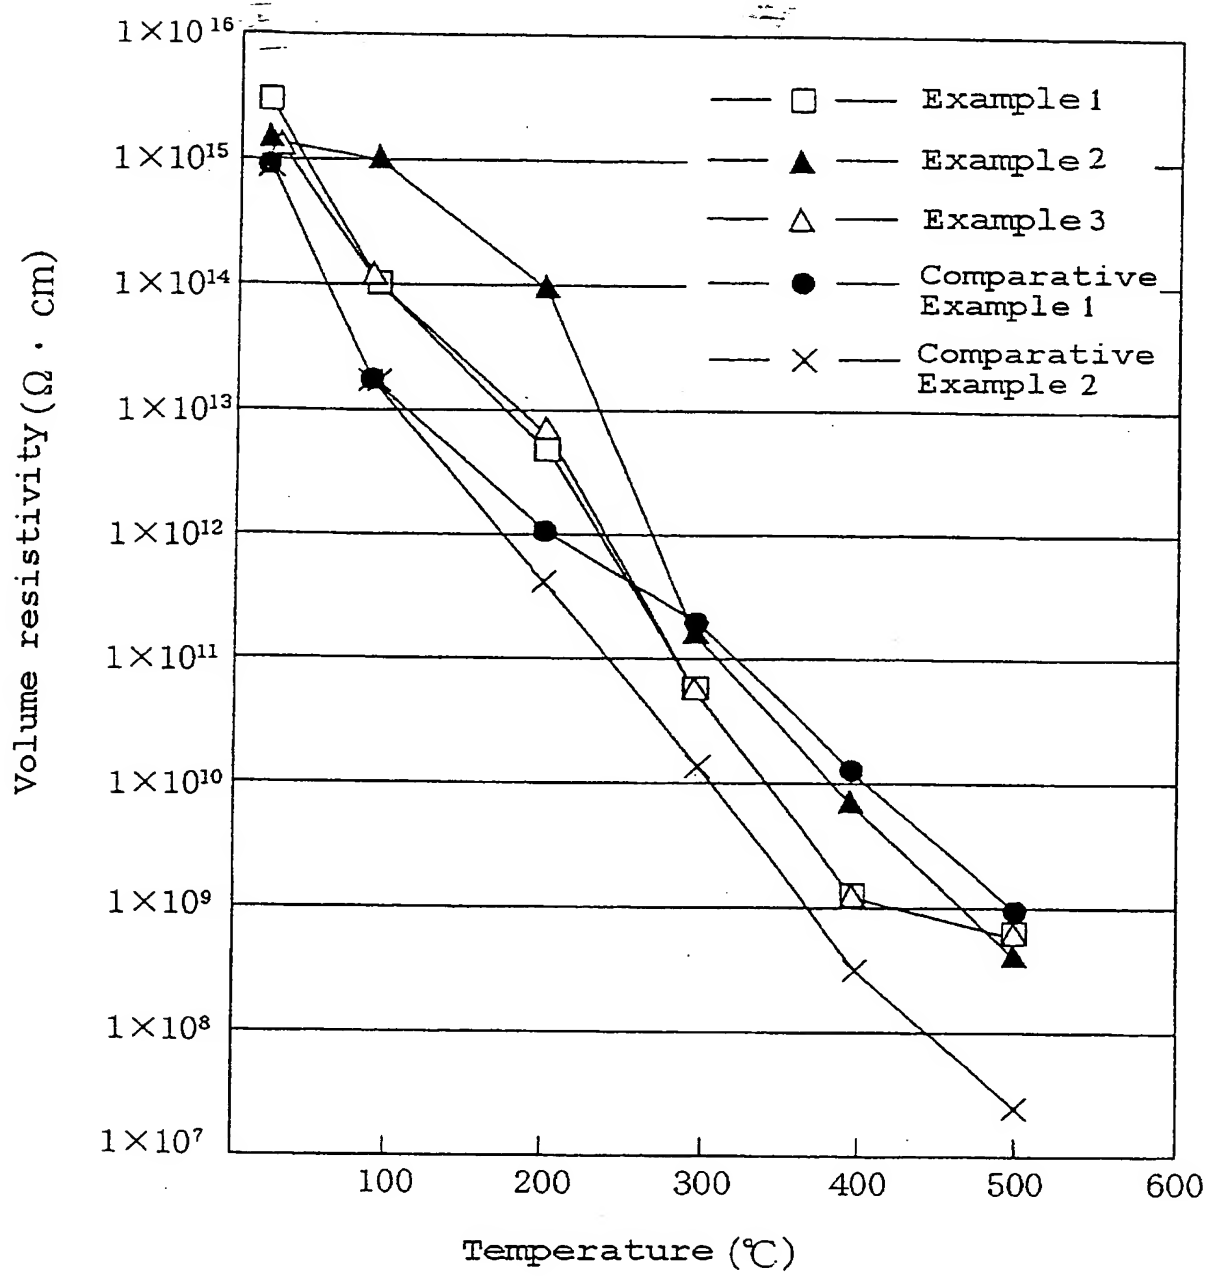

2 / 16

Fig. 2

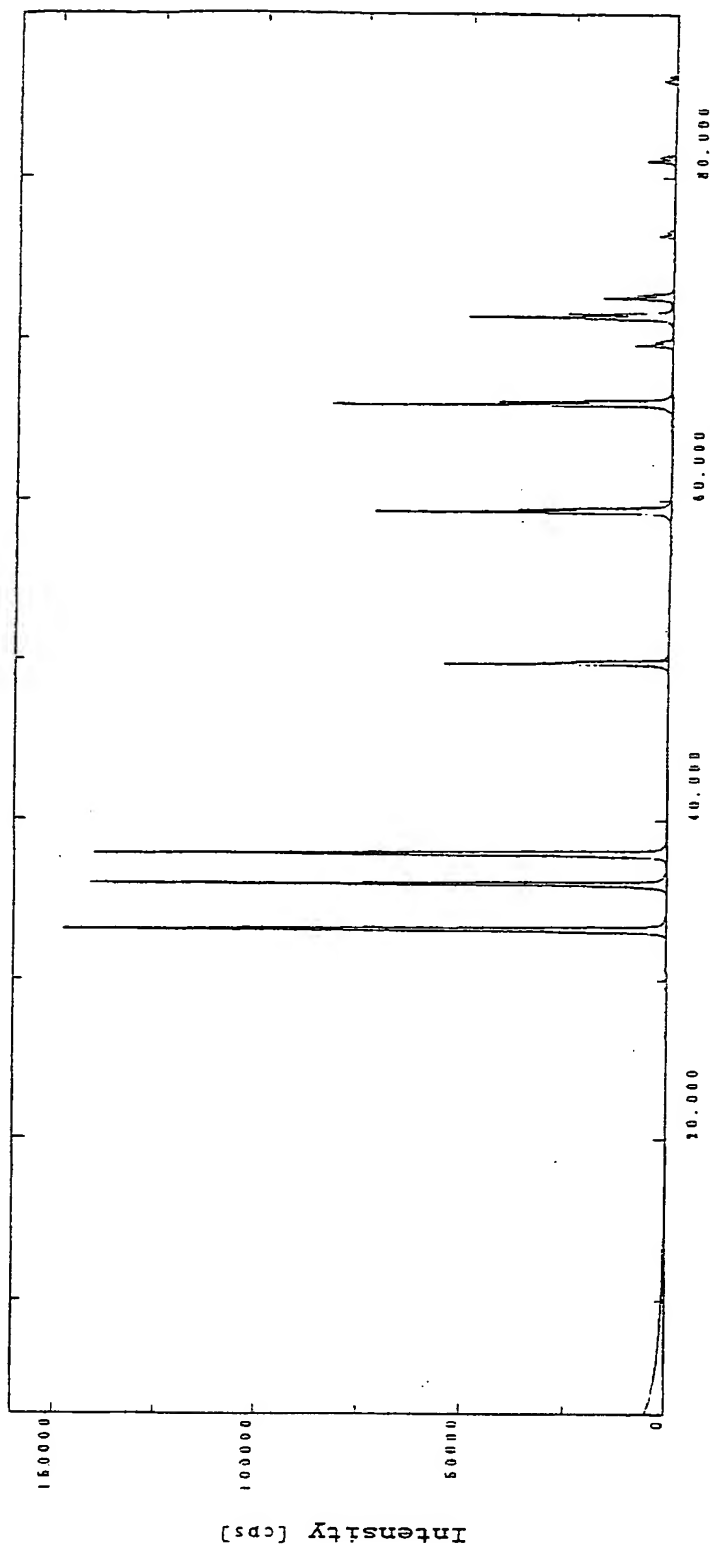


2 θ [°]

Sample name : Outside	X-rays : Cu K-ALPHA/ 50 kv/ 300 mA	Counter : Scintillation counter
File : T990603.0339	Goniometer : RINT 2000 wide angle goniometer	Scanning mode : Continuous
Comments : Wide angle measurement	Attachment : Standard sample holder	Scanning speed : 2.000 °/min.
Date of measurement : 03-Jun-99 15:59	Filter : Not used	Scanning step : 0.020 °
Measurer : R I N T	Incident monochrome : Full automatic monochromator	Scanning axis : 2 θ / θ
	Divergent slit : "1deg."	Scanning range : 3.000 ~ 90.000 °
	scattering slit : "1deg."	θ offset : 0.000 °
	Light-receiving slit : "0.3mm"	


3 / 16

Fig. 3

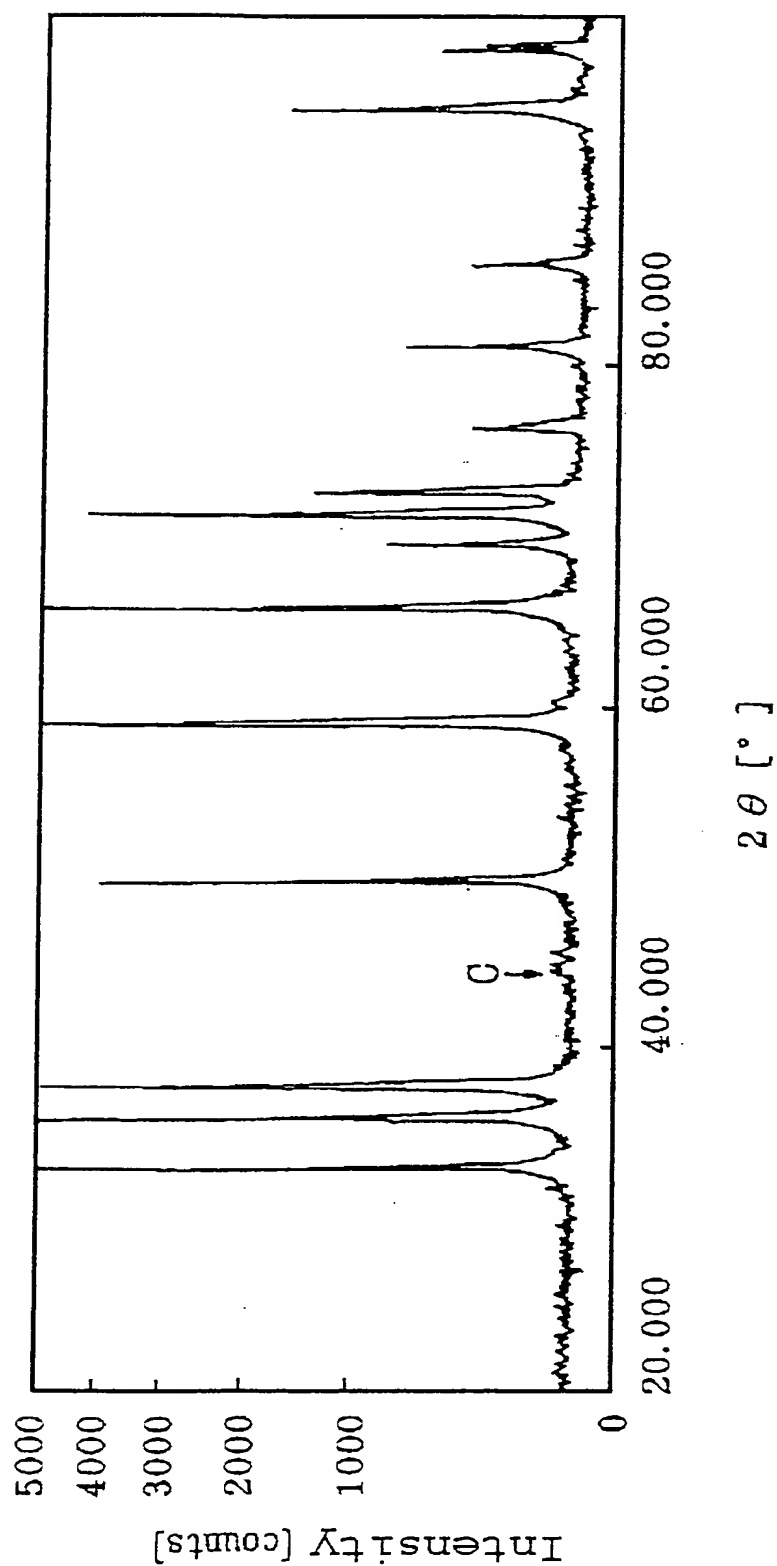


4 / 16

Fig. 4

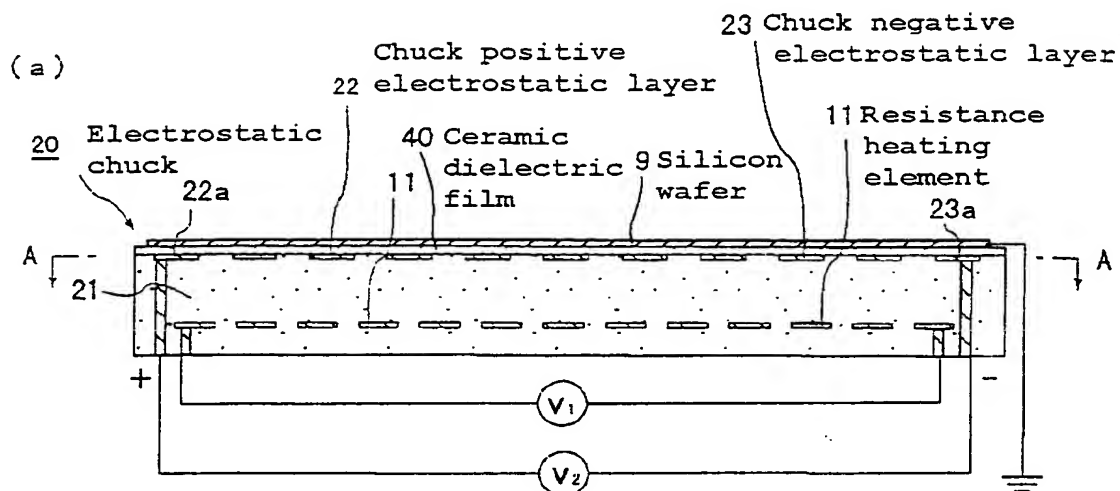


(b)

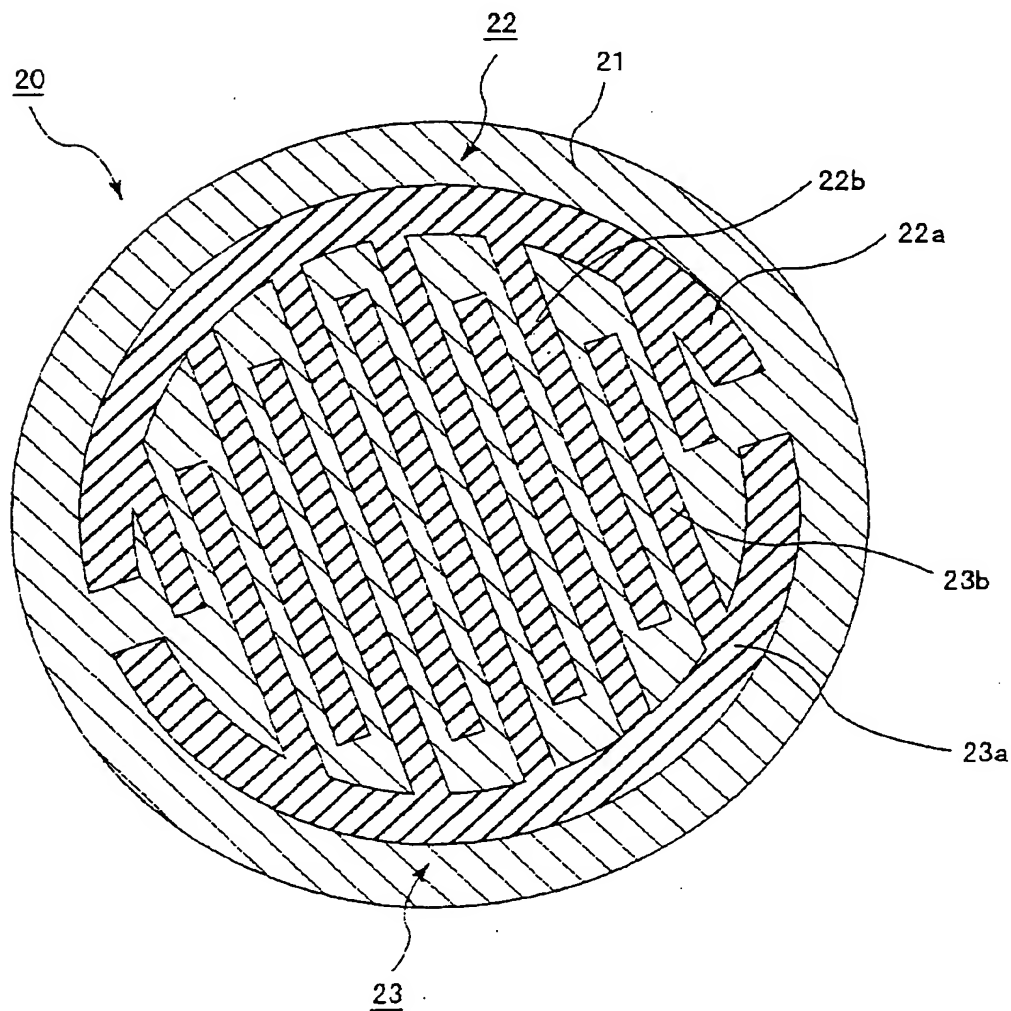


5/16

Fig. 5

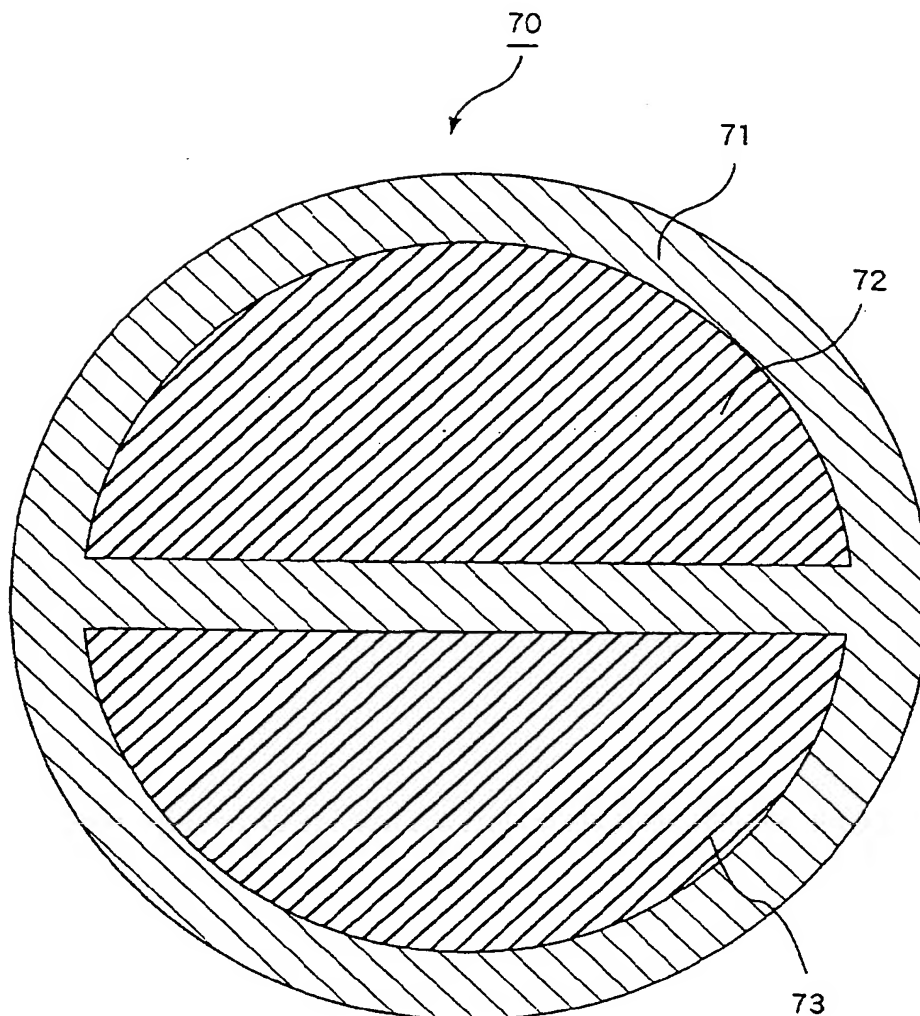


6 / 16

Fig. 6

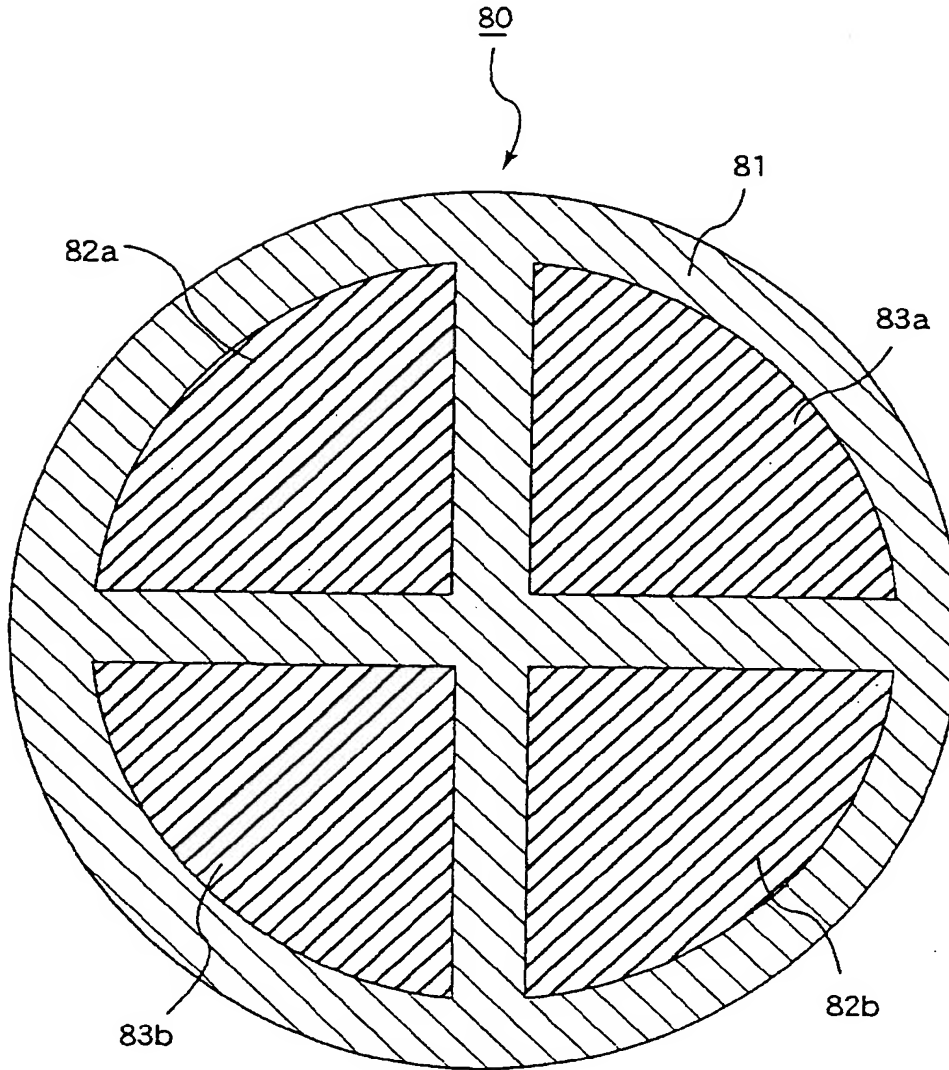


7 / 16

Fig. 7

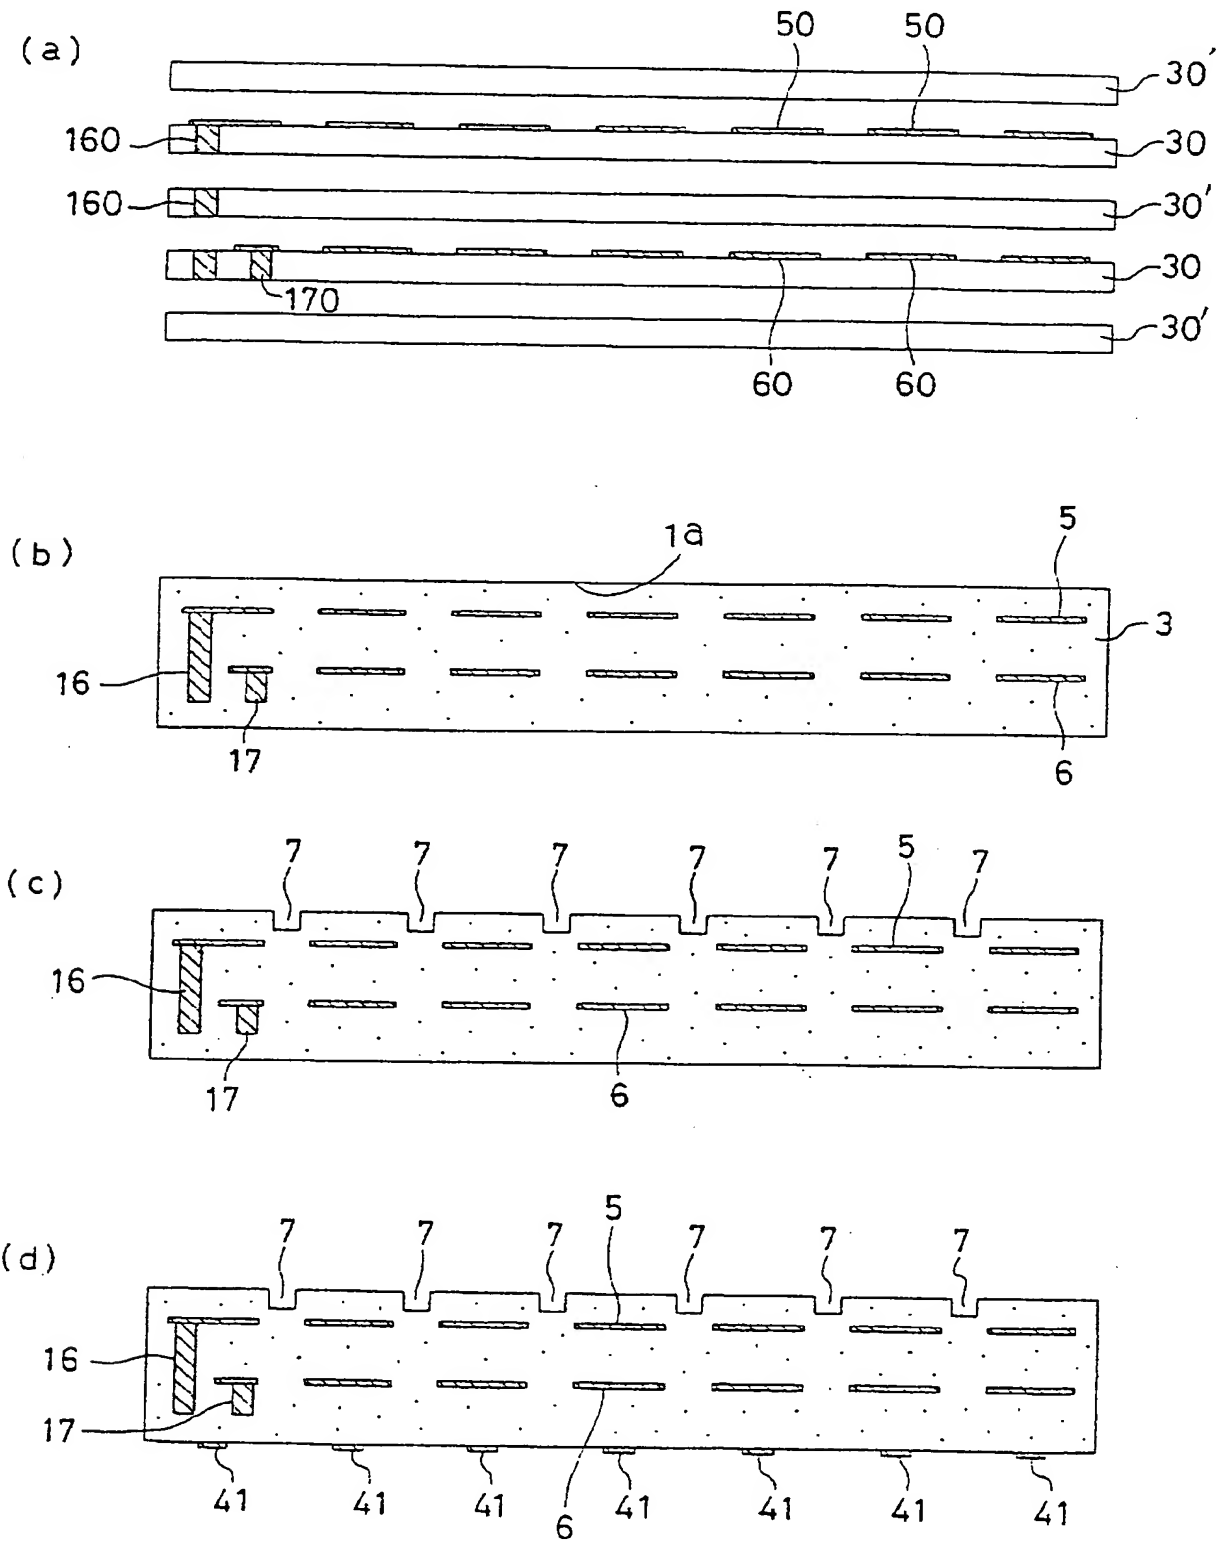


8 / 16

Fig. 8

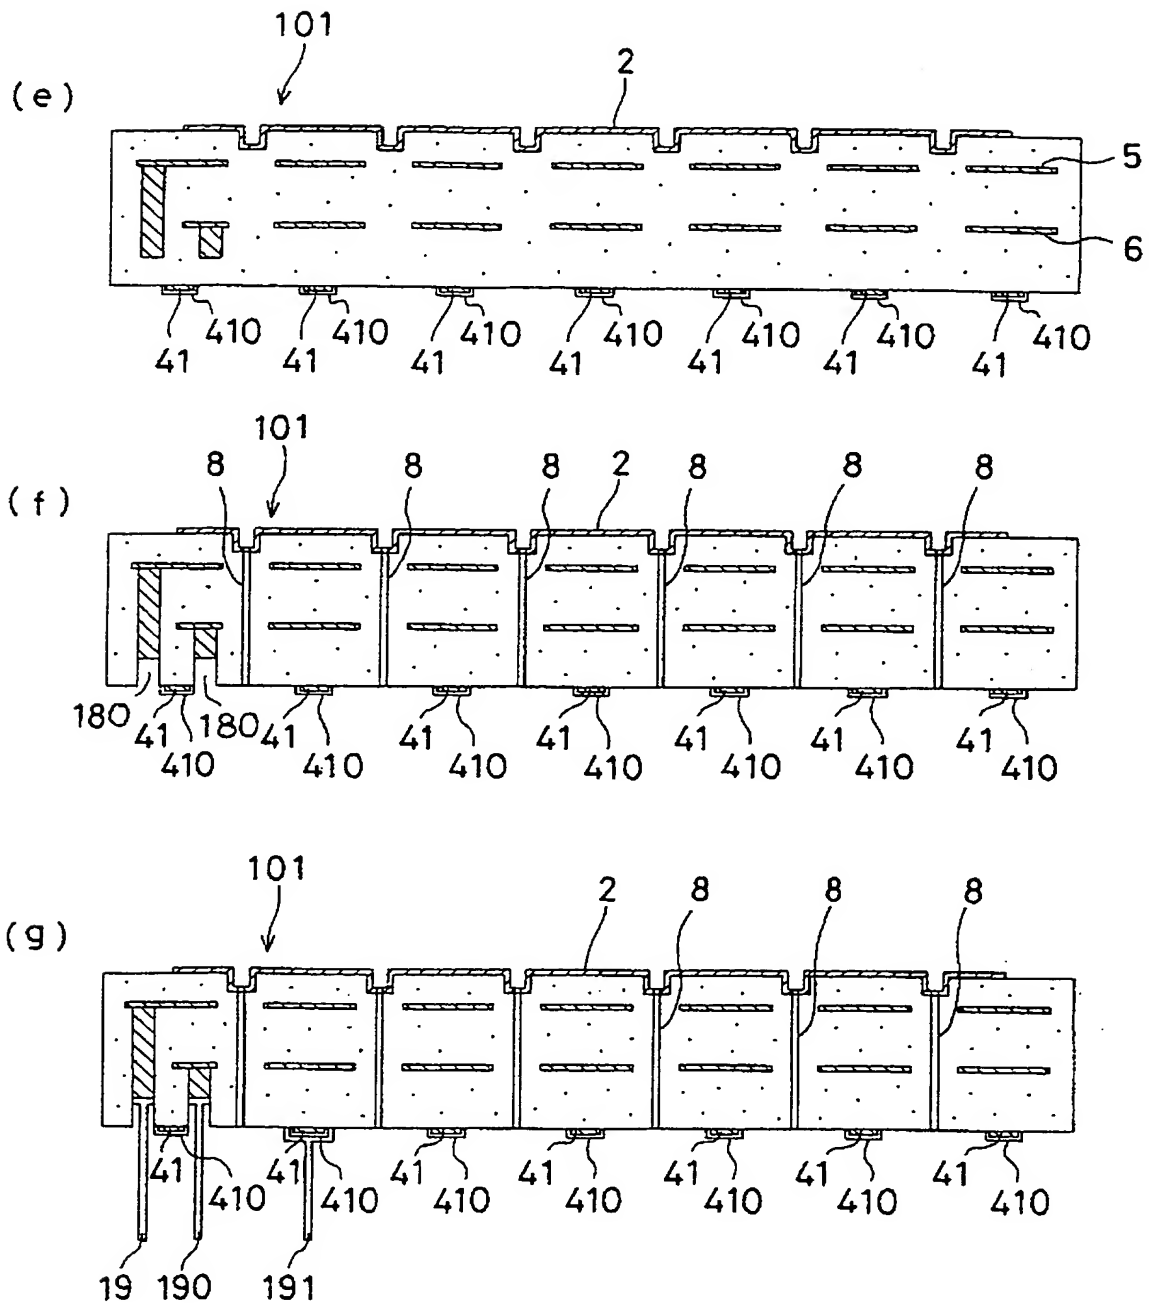


9 / 16

Fig. 9

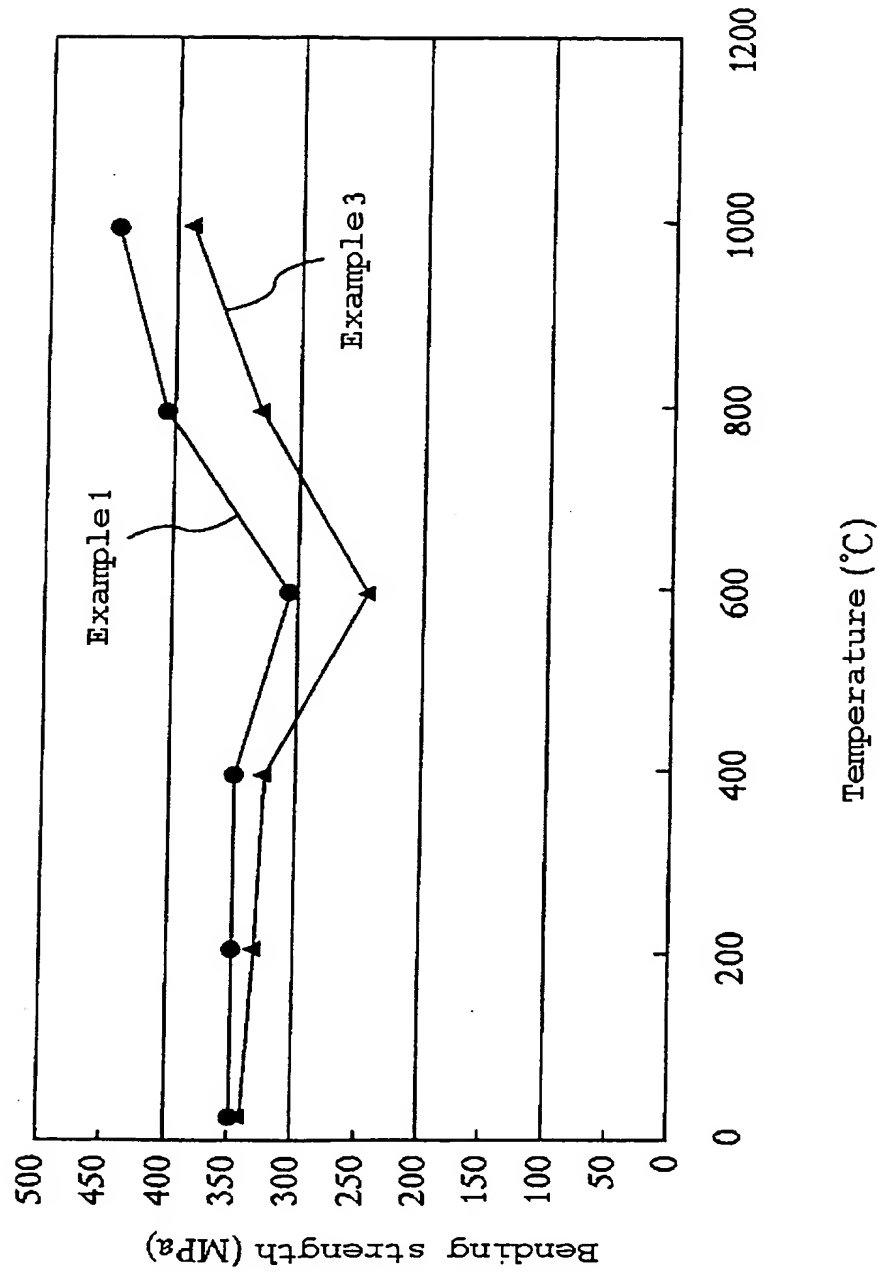


10/16

Fig. 10

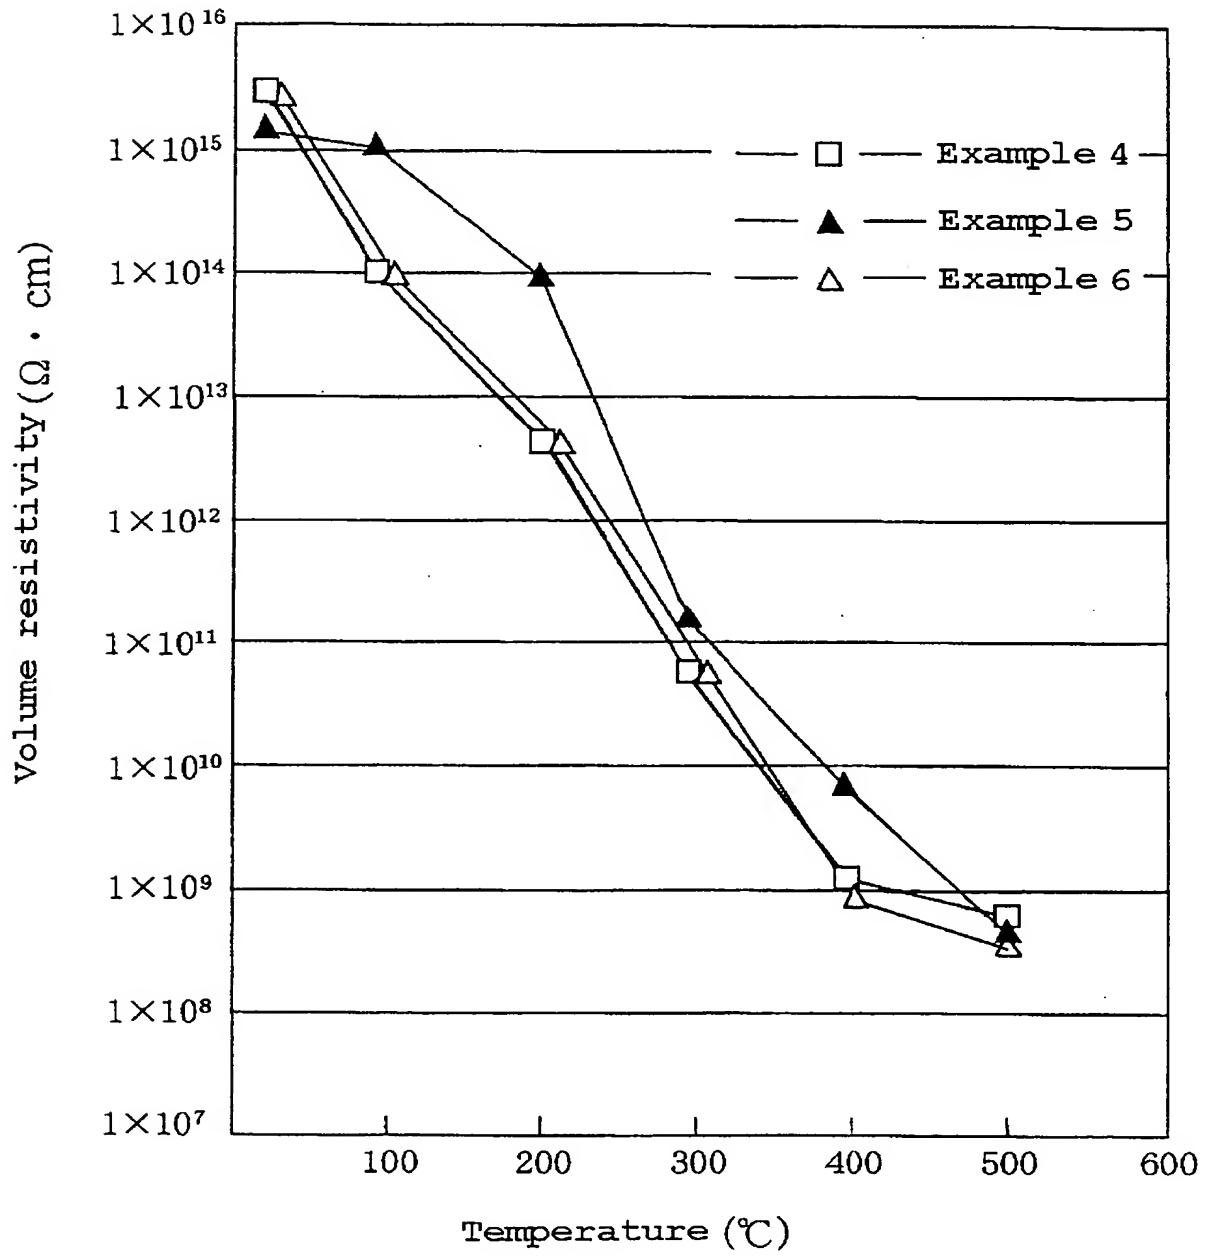


11 / 16

Fig. 11

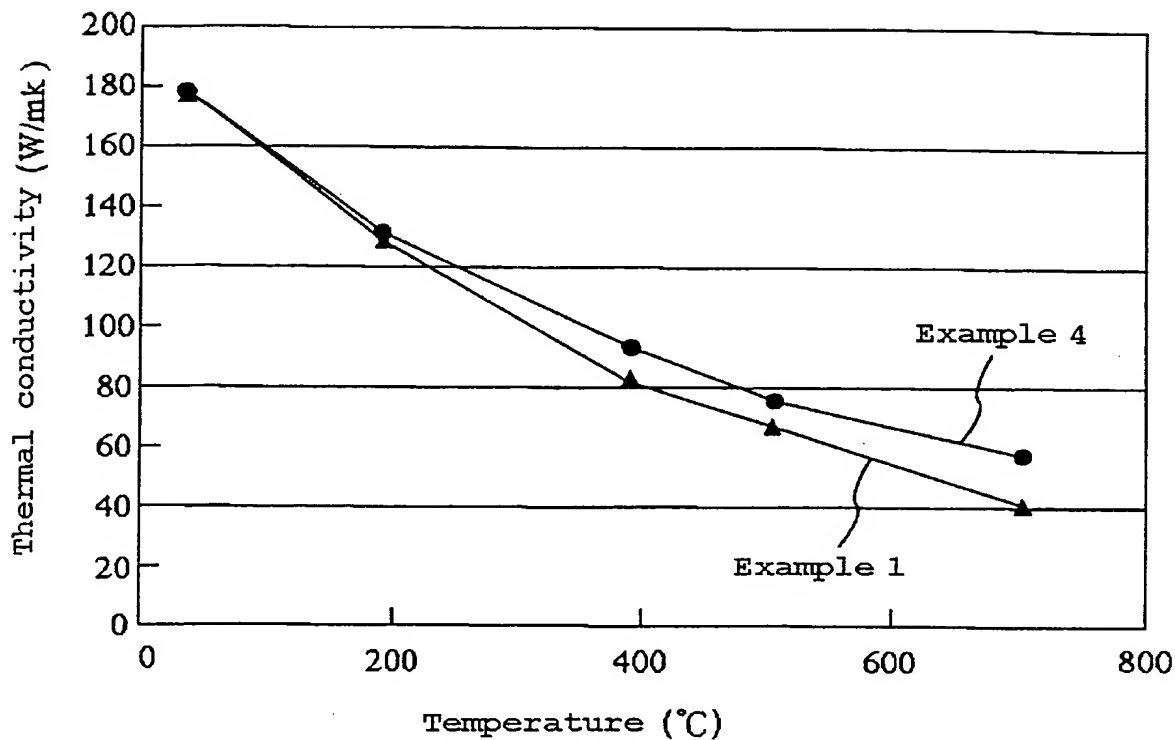

12 / 16


Fig. 12

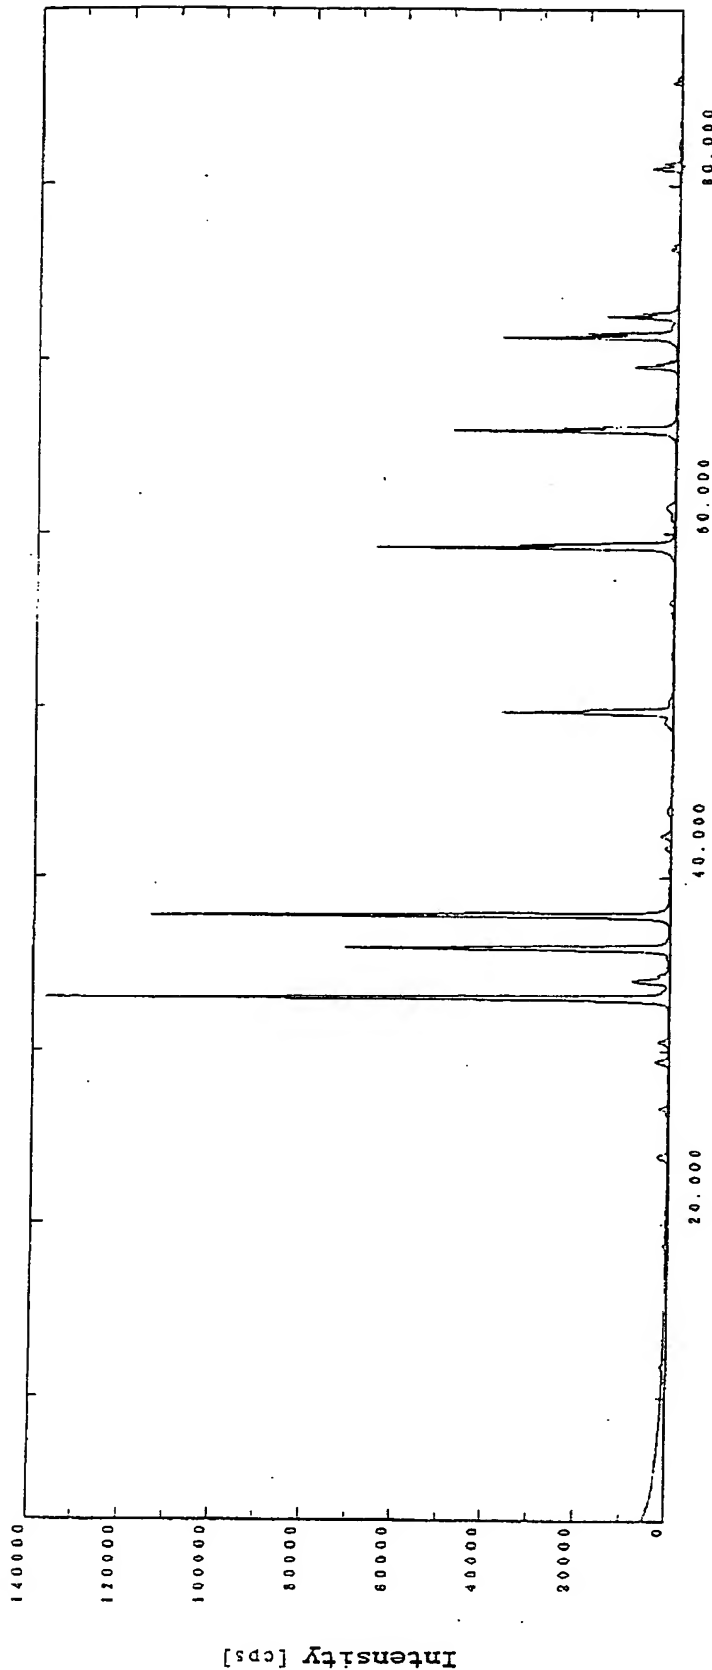

Sample name : Inside	I-rays : Cu K-ALPHA1 / 50 kV / 300 mA	Counter: Scintillation counter
File : T990603.0340	Goniometer : RINT 2000 wide angle goniometer	Scanning mode: Continuous
Comments : Wide angle measurement	Attachment : Standard sample holder	Scanning speed: 2000° /min.
Date of measurement : 03-Jun-99 16:50	Filter : Not used	Scanning step: 0.020°
Measurer : R J N T	Incident monochrome	Scanning axis: 2θ / θ
	Counter monochromator: Full automatic monochromator	Scanning range: 3.000-90.000°
	Divergent slit : "1deg."	θ offset: 0.000°
	scattering slit : "1deg."	
	Light-receiving slit : "0.3mm"	

13 / 16

Fig. 13

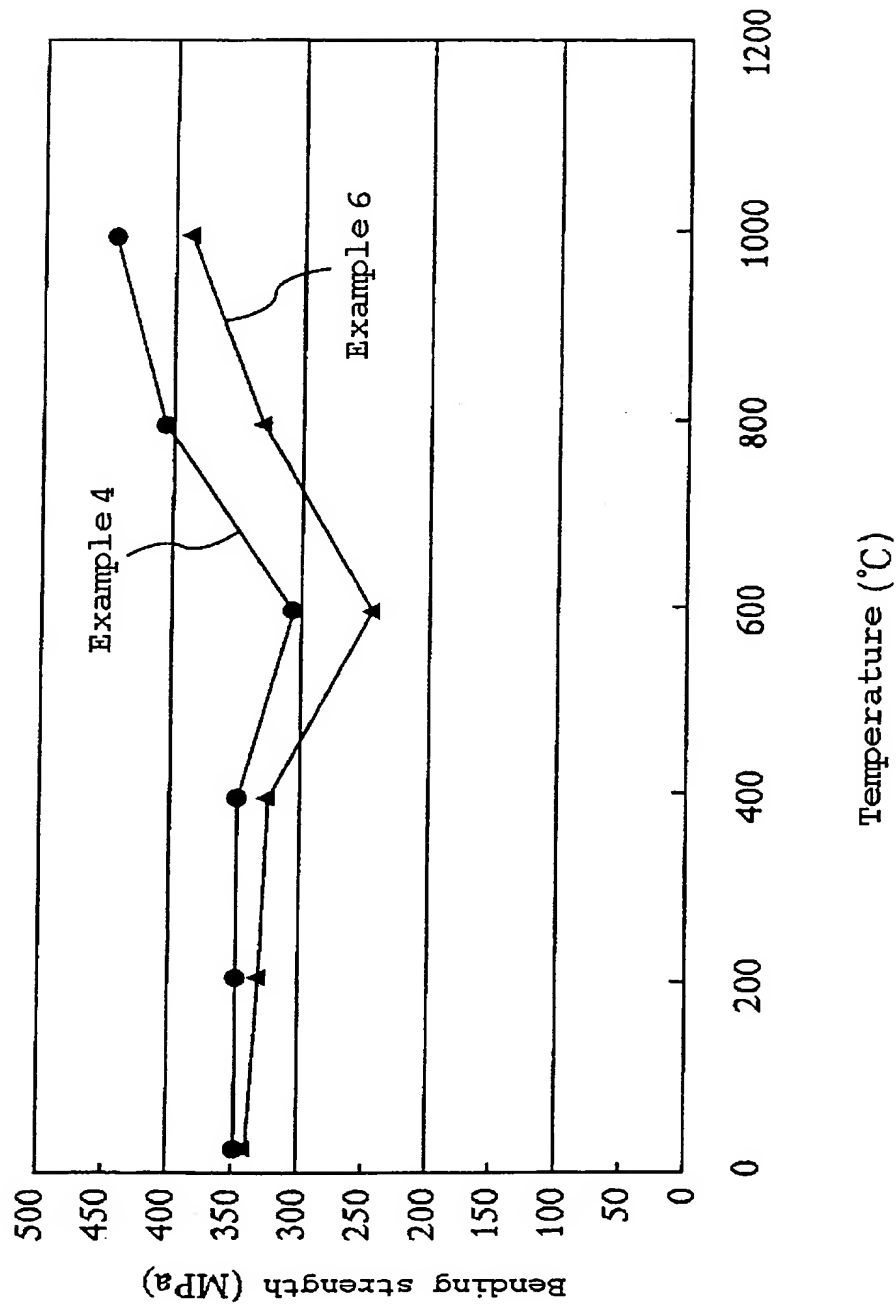

14/16

Fig. 14

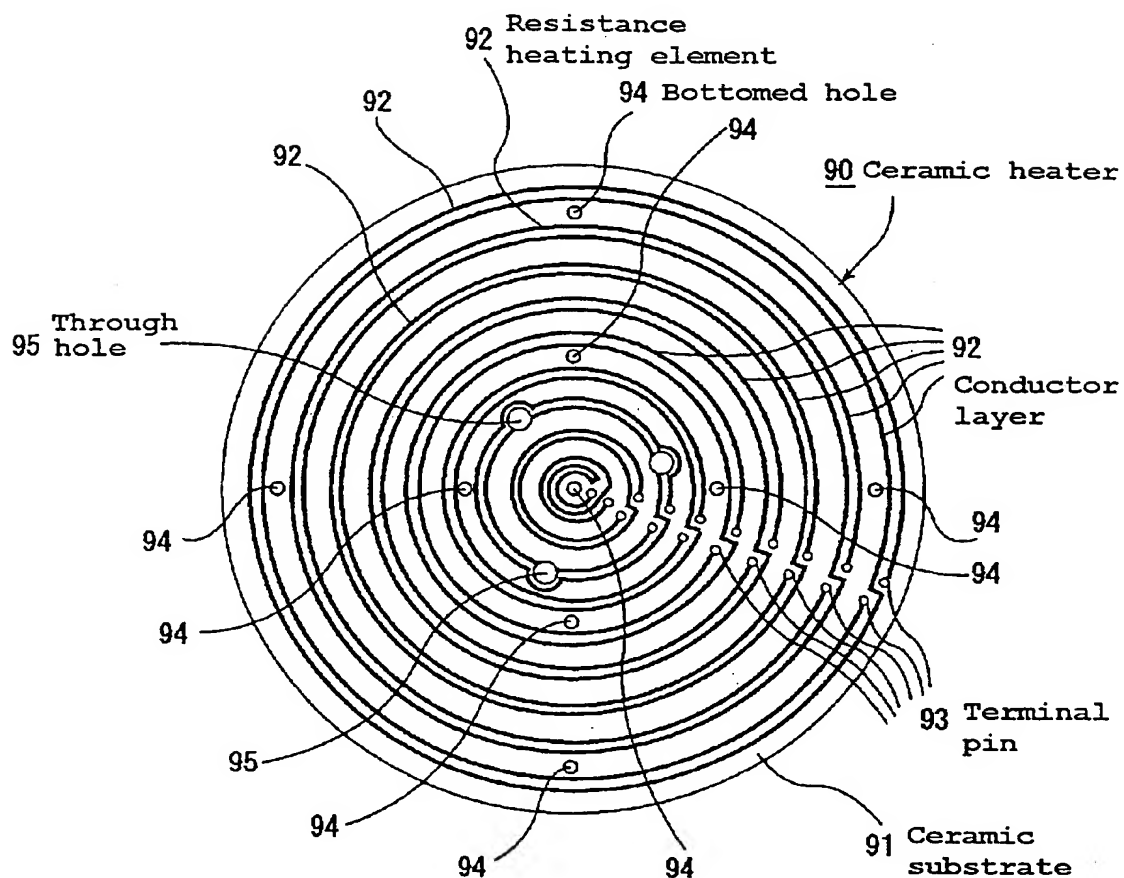


Fig. 15

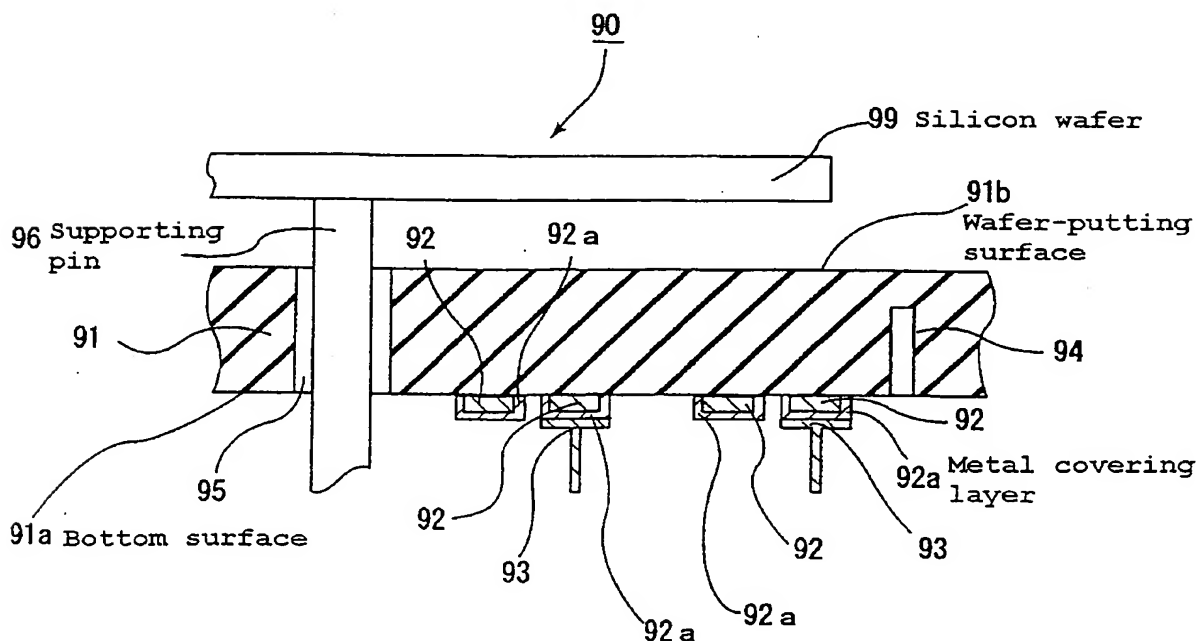


Fig. 16


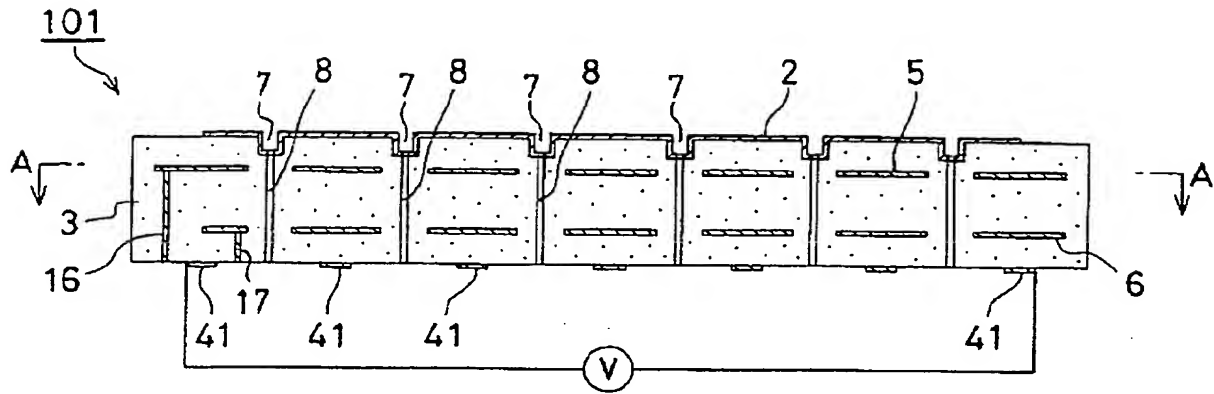


Fig. 17



16/16

Fig. 18

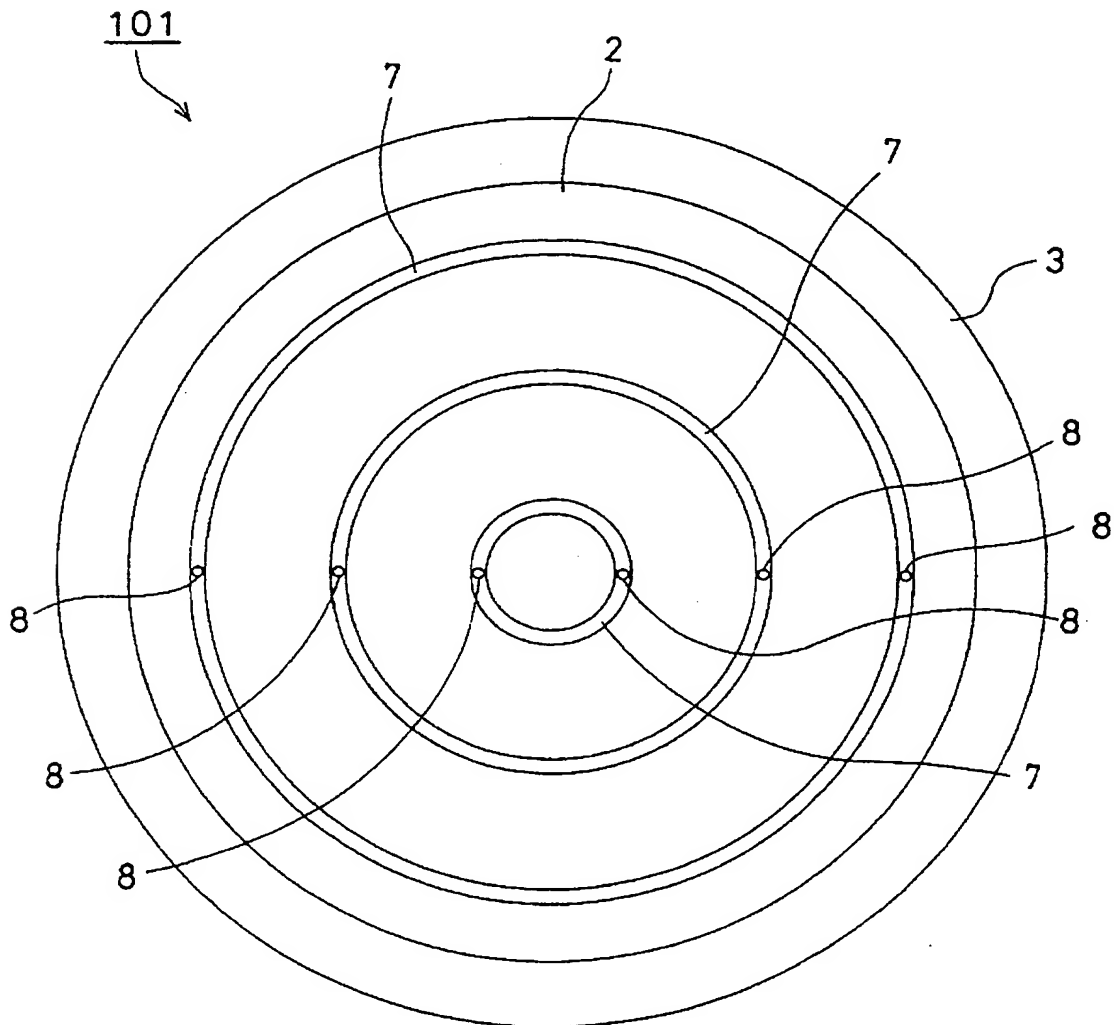